

# Air Monitoring Summary Tables

The table below summarizes monitoring data collected using the H<sub>2</sub>S analyzers deployed at the onsite stations. All times in Eastern Standard Time (EST).

**From:** 10/11/24 12:00 am

**To:** 10/11/24 11:59 pm

## Onsite Fenceline Monitors

Instrument	Analyte	30-min AEGL Reached?	Concentration Range Detected <sup>a</sup>	24-hr Average <sup>a</sup>	7-day Average	30-min AEGL
<b>Station 1</b>						
TAPI Analyzer	H <sub>2</sub> S	No	0 – 43 ppb	6.48 ppb <sup>b</sup>	6.67 ppb	600 ppb
<b>Station 2</b>						
TAPI Analyzer	H <sub>2</sub> S	No	0 – 1 ppb	0.27 ppb <sup>c</sup>	0.23 ppb	600 ppb
<b>Station 3</b>						
TAPI Analyzer	H <sub>2</sub> S	No	0 – 1 ppb	0.25 ppb	0.25 ppb	600 ppb

<sup>a</sup> Based on 30-minute averages.


<sup>b</sup> The 24-hour H<sub>2</sub>S average at Station 1 from the start of the sampling period to the end of the sampling period is represented by the backup unit data.


<sup>c</sup> The 24-hour H<sub>2</sub>S average at Station 2 from the start of the sampling period to the end of the sampling period is represented by the backup unit data

### Notes:




ATSDR MRL	Agency for Toxic Substances and Disease Registry Minimal Risk Level (MRL)
AEGL	EPA Acute Exposure Guidelines Levels
H <sub>2</sub> S	Hydrogen Sulfide
TAPI	Teledyne API H <sub>2</sub> S Analyzer
hr	Hour
min	Minute
ppb	Parts per billion
MRL Limit	Limit defined as a 14-day average value

**Station 1 Wind Rose – Shows the direction the wind is coming from, the monitoring station being at the center of the rose.**

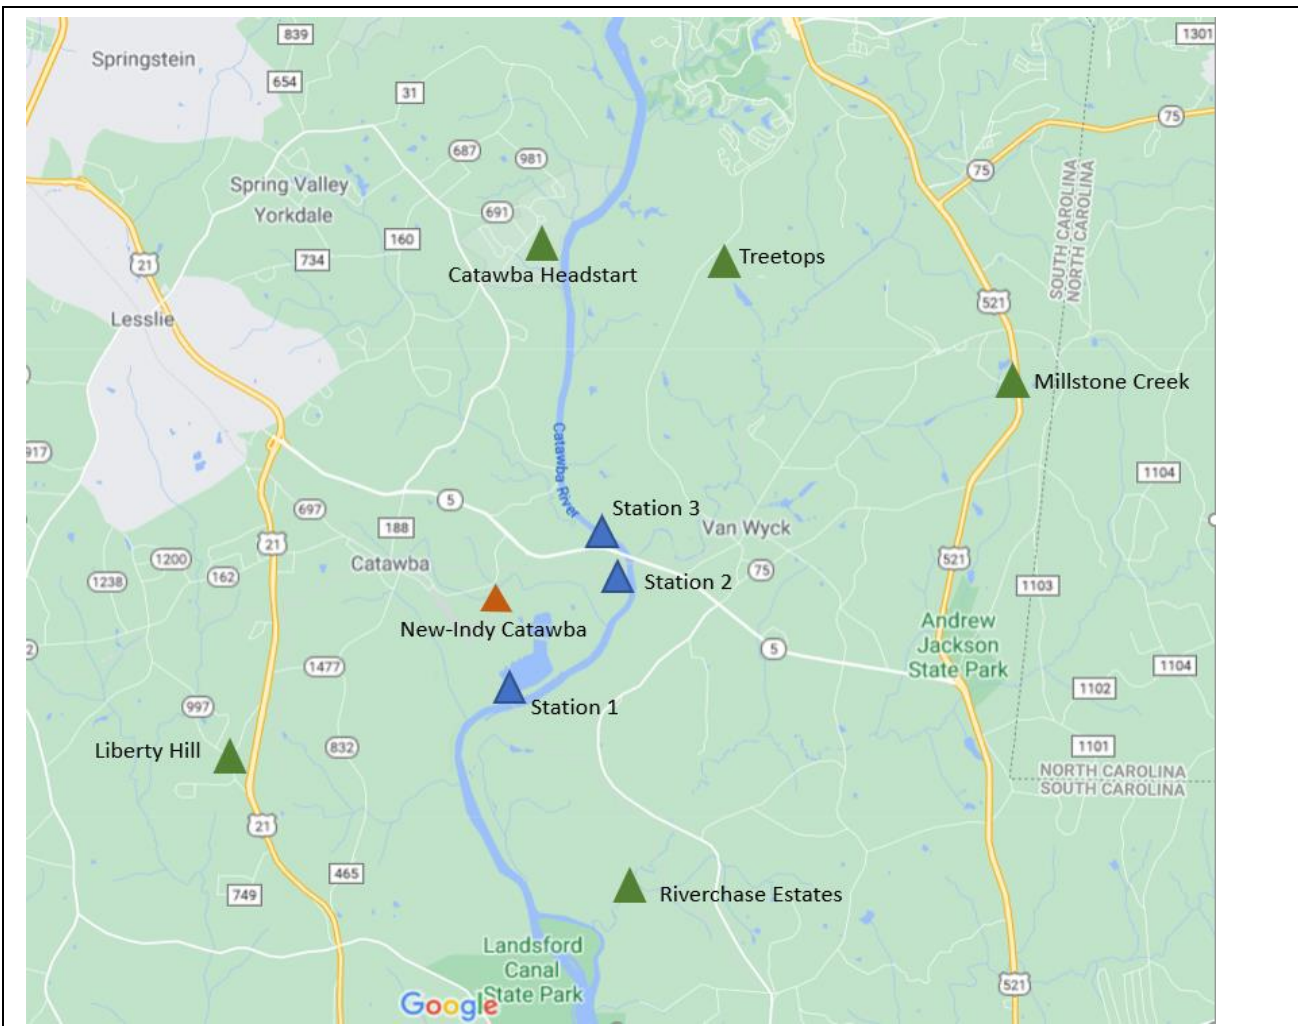



**Legend**

-  Offsite Fixed Monitoring Locations
-  Onsite Fixed Monitoring Locations
-  New-Indy Catawba



## Period H<sub>2</sub>S Monitoring Hydrogen Sulfide Onsite Monitors

Below are graphs for onsite locations during the current reporting period.


Depending on wind direction, the H<sub>2</sub>S measured at the onsite fence line locations may not exit the mill property at reported concentrations. Wind directions from offsite locations, blowing onto mill property, will disperse ambient concentrations to lower levels prior to exiting the plant site.

Winds were predominantly coming from the north-northeast, northeast, south, and south-southeast direction throughout the day at 1 to 7 mph.

See wind rose diagram with aerial map figure for full wind data during this reporting period.



### Station3 - 10/11/2024



Submitted Fenceline H<sub>2</sub>S and Met 30-minute Data

30-Minute Avgs	Station 1			Station 2			Station 3		
	H2S	Met		H2S	Met		H2S	Met	
	30min Avg H2S Conc.	30min Avg WS	30min Avg WD	30min Avg H2S Conc.	30min Avg WS	30min Avg WD	30min Avg H2S Conc.	30min Avg WS	30min Avg WD
Date / Time	ppb	mph	degrees	ppb	mph	degrees	ppb	mph	degrees
10/11/2024 0:30	AX	2.4	54	0.2	0.3	31	0.2	0.2	289
10/11/2024 1:00	2.2	3.6	41	AX	0.5	27	0.2	0.2	314
10/11/2024 1:30	6.3	3.2	43	0.2	0.4	38	AX	0.3	339
10/11/2024 2:00	4.7	2.3	54	0.2	0.4	41	0.2	0.2	292
10/11/2024 2:30	7.7	1.5	48	0.2	0.4	41	0.2	0.2	288
10/11/2024 3:00	13.2	2.3	48	0.2	0.5	17	0.2	0.2	270
10/11/2024 3:30	12.5	2.8	45	0.2	0.5	24	0.2	0.4	301
10/11/2024 4:00	8.1	3.7	43	0.2	0.5	26	0.2	0.6	322
10/11/2024 4:30	23.6	3.2	33	0.2	0.6	44	0.2	0.9	358
10/11/2024 5:00	40.4	2.6	36	0.2	0.6	47	0.2	0.4	40
10/11/2024 5:30	4.8	4.1	48	0.2	0.8	48	0.2	0.7	2
10/11/2024 6:00	9.4	3.1	39	0.2	0.5	45	0.2	0.2	292
10/11/2024 6:30	39.8	1.3	10	0.2	0.5	38	0.2	0.2	293
10/11/2024 7:00	43.0	1.5	24	0.2	0.5	34	0.2	0.4	354
10/11/2024 7:30	36.6	3.5	34	0.2	0.7	31	0.2	0.9	14
10/11/2024 8:00	14.0	5.1	28	0.2	0.6	345	0.2	2.2	359
10/11/2024 8:30	15.0	3.3	9	0.2	0.6	11	0.2	2.7	359
10/11/2024 9:00	9.9	5.0	33	0.2	1.8	7	0.2	1.4	16
10/11/2024 9:30	2.8	6.1	34	0.2	2.6	7	0.2	2.7	21
10/11/2024 10:00	2.1	4.1	53	0.2	1.5	35	0.2	2.0	59
10/11/2024 10:30	0.2	6.2	60	0.2	1.9	96	0.2	3.4	56
10/11/2024 11:00	0.2	7.2	47	0.2	1.6	64	0.2	2.7	47
10/11/2024 11:30	0.2	6.3	21	0.2	1.8	101	0.2	2.9	33
10/11/2024 12:00	0.2	2.7	12	0.2	1.8	73	0.2	2.0	352
10/11/2024 12:30	0.2	3.4	62	0.2	2.1	40	0.2	1.7	46
10/11/2024 13:00	0.2	3.5	118	0.2	2.3	169	0.2	1.7	26
10/11/2024 13:30	0.2	2.1	178	0.2	2.1	109	0.2	1.9	276
10/11/2024 14:00	0.2	2.4	156	0.2	2.4	311	0.2	1.4	297
10/11/2024 14:30	0.2	3.2	71	0.2	3.0	290	0.2	1.6	236
10/11/2024 15:00	0.2	3.2	46	0.2	2.7	292	0.2	1.8	35
10/11/2024 15:30	0.6	2.3	41	0.2	2.2	352	0.2	1.7	42
10/11/2024 16:00	0.8	2.3	55	0.2	2.0	312	0.2	0.7	271
10/11/2024 16:30	1.3	3.5	28	0.2	2.0	351	0.2	0.4	295
10/11/2024 17:00	0.7	1.6	102	0.2	0.4	77	0.2	0.5	200
10/11/2024 17:30	0.2	1.8	168	0.2	0.2	72	0.2	0.3	228
10/11/2024 18:00	0.2	2.6	179	0.2	0.3	280	0.2	0.4	262
10/11/2024 18:30	0.2	1.9	178	0.2	0.2	49	0.2	0.3	305
10/11/2024 19:00	0.2	2.0	182	0.2	0.2	24	0.2	0.3	207
10/11/2024 19:30	0.2	1.2	183	0.2	0.3	350	0.2	0.3	301
10/11/2024 20:00	0.2	1.5	162	0.2	0.2	19	0.2	0.2	280
10/11/2024 20:30	0.2	1.1	160	0.2	0.2	19	0.2	0.2	293
10/11/2024 21:00	0.2	1.3	161	0.4	0.2	26	0.2	0.2	268
10/11/2024 21:30	0.2	1.4	167	0.7	0.2	23	0.5	0.2	271
10/11/2024 22:00	0.2	1.2	153	1.1	0.3	16	0.8	0.2	18
10/11/2024 22:30	0.2	1.5	156	0.6	0.2	33	1.3	0.2	293
10/11/2024 23:00	0.2	1.6	171	0.9	0.2	25	0.8	0.2	341
10/11/2024 23:30	0.2	1.3	182	0.8	0.2	9	0.2	0.2	72
10/12/2024 0:00	0.2	2.2	190	0.2	0.2	324	0.2	0.2	289

AQS Null Data Codes	
Qualifier Code	Item Description
AB	TECHNICIAN UNAVAILABLE
AC	CONSTRUCTION/REPAIRS IN AREA
AD	SHELTER STORM DAMAGE
AE	SHELTER TEMPERATURE OUTSIDE LIMITS
AI	INSUFFICIENT DATA (CAN'T CALCULATE)
AM	MISCELLANEOUS VOID
AN	MACHINE MALFUNCTION
AO	BAD WEATHER
AP	VANDALISM
AS	POOR QUALITY ASSURANCE RESULTS
AT	CALIBRATION
AU	MONITORING WAIVED
AV	POWER FAILURE (POWR)
AW	WILDLIFE DAMAGE
AX	PRECISION CHECK (PREC)
AY	Q C CONTROL POINTS (ZERO/SPAN)
AZ	Q C AUDIT (AUDT)
BA	MAINTENANCE/ROUTINE REPAIRS
BB	UNABLE TO REACH SITE
BC	MULTI-POINT CALIBRATION
BD	AUTO CALIBRATION
BE	BUILDING/SITE REPAIR
BF	PRECISION/ZERO/SPAN
BJ	OPERATOR ERROR
BK	SITE COMPUTER/DATA LOGGER DOWN
EC	EXCEED CRITICAL CRITERIA