

Air Monitoring Summary Tables

The table below summarizes monitoring data collected using the H₂S analyzers deployed at the onsite stations.
All times in Eastern Standard Time (EST).

From: 12/08/24 12:00 am

To: 12/08/24 11:59 pm

Onsite Fenceline Monitors

Instrument	Analyte	30-min AEGL Reached?	Concentration Range Detected ^a	24-hr Average ^a	7-day Average	30-min AEGL
Station 1						
TAPI Analyzer	H ₂ S	No	0 – 3 ppb	0.39 ppb ^b	1.05 ppb	600 ppb
Station 2						
TAPI Analyzer	H ₂ S	No	0 – 7 ppb	0.81 ppb ^c	0.41 ppb	600 ppb
Station 3						
TAPI Analyzer	H ₂ S	No	0 – 3 ppb	0.99 ppb	0.48 ppb	600 ppb

^a Based on 30-minute averages.


^b The 24-hour H₂S average at Station 1 from the start of the sampling period to the end of the sampling period is represented by the backup unit data.

^c The 24-hour H₂S average at Station 2 from the start of the sampling period to the end of the sampling period is represented by the backup unit data

Notes:

ATSDR MRL	Agency for Toxic Substances and Disease Registry Minimal Risk Level (MRL)
AEGL	EPA Acute Exposure Guidelines Levels
H ₂ S	Hydrogen Sulfide
TAPI	Teledyne API H ₂ S Analyzer
hr	Hour
min	Minute
ppb	Parts per billion
MRL Limit	Limit defined as a 14-day average value

Station 1 Wind Rose – Shows the direction the wind is coming from, the monitoring station being at the center of the rose.

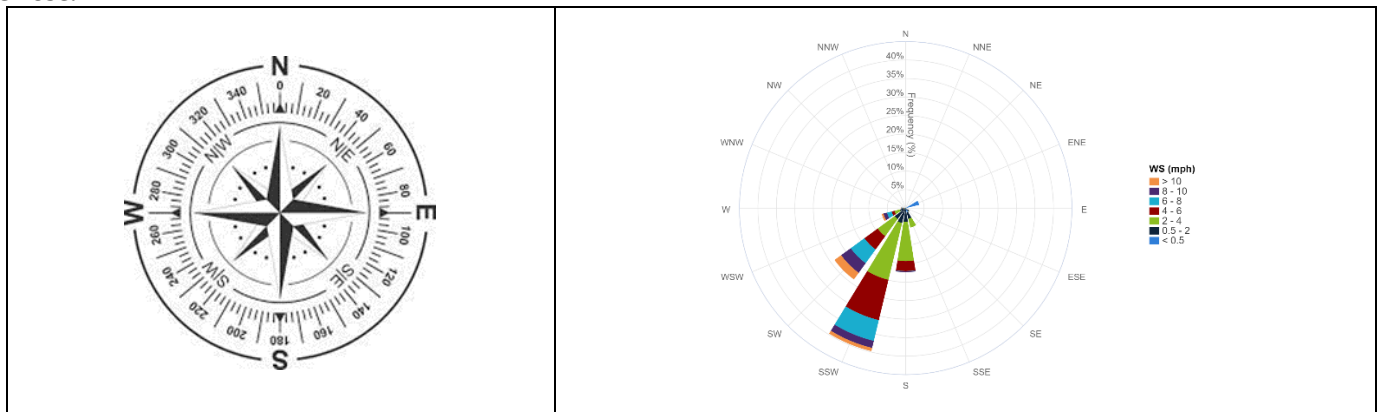



Legend



Onsite Fixed Monitoring Locations



New-Indy Catawba



Period H₂S Monitoring Hydrogen Sulfide Onsite Monitors

Below are graphs for onsite locations during the current reporting period.


Depending on wind direction, the H₂S measured at the onsite fence line locations may not exit the mill property at reported concentrations. Wind directions from offsite locations, blowing onto mill property, will disperse ambient concentrations to lower levels prior to exiting the plant site.

Winds were predominantly coming from the southwest, south-southwest, and south direction throughout the day at 0 to 10 mph.

See wind rose diagram with aerial map figure for full wind data during this reporting period.

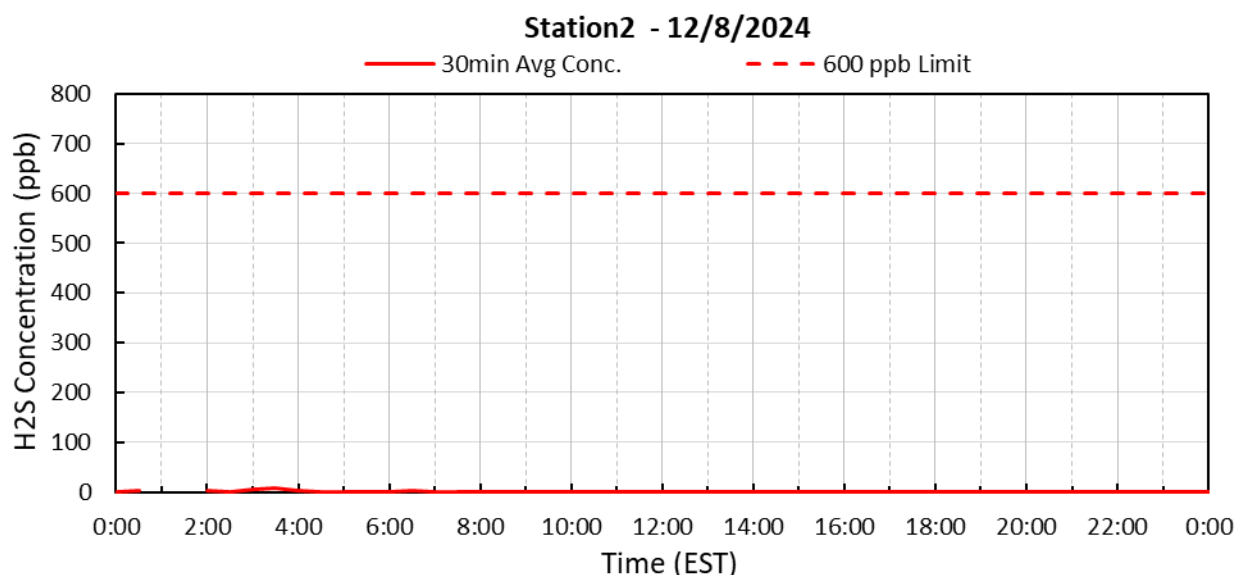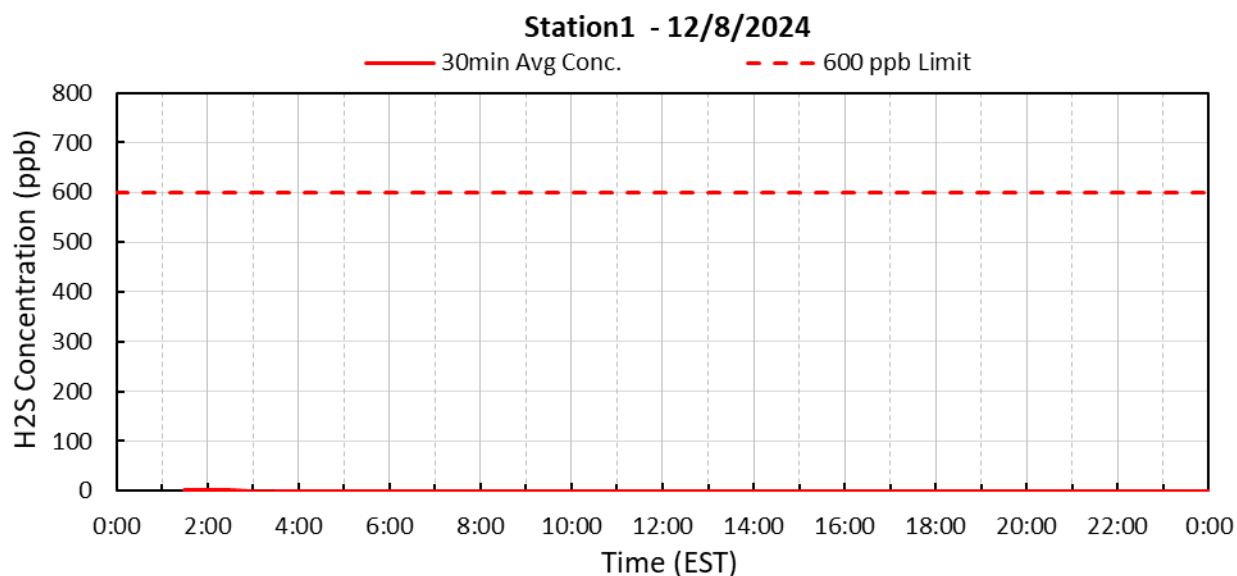

Station3 - 12/8/2024

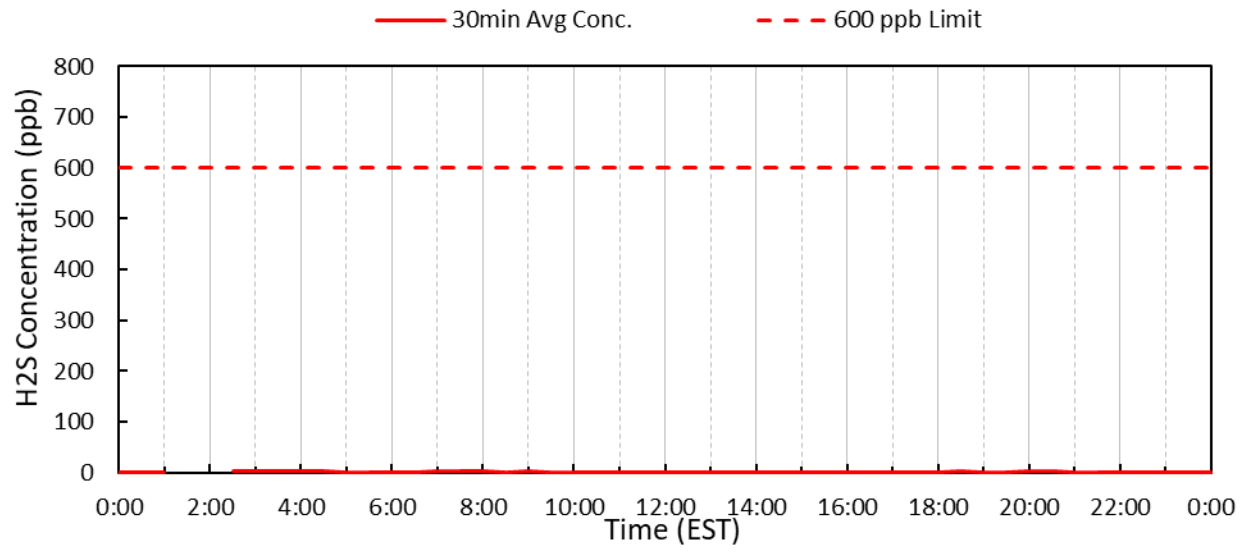

Submitted Fenceline H₂S and Met 30-minute Data

30-Minute Avgs	Station 1			Station 2			Station 3		
	H2S	Met		H2S	Met		H2S	Met	
	30min Avg H2S Conc.	30min Avg WS	30min Avg WD	30min Avg H2S Conc.	30min Avg WS	30min Avg WD	30min Avg H2S Conc.	30min Avg WS	30min Avg WD
Date / Time	ppb	mph	degrees	ppb	mph	degrees	ppb	mph	degrees
12/8/2024 0:30	BF	3.8	223	1.9	1.3	60	0.9	1.8	159
12/8/2024 1:00	BF	2.0	247	BF	1.1	84	0.2	1.3	155
12/8/2024 1:30	3.3	2.8	208	BF	1.1	186	BF	2.0	177
12/8/2024 2:00	1.9	2.1	211	2.1	0.6	231	BF	1.1	190
12/8/2024 2:30	1.1	2.9	214	0.9	1.2	210	3.1	1.2	193
12/8/2024 3:00	0.8	3.0	213	5.8	1.9	215	2.2	0.6	185
12/8/2024 3:30	0.6	2.0	207	7.1	1.9	240	2.3	0.7	199
12/8/2024 4:00	0.5	2.3	204	2.5	1.6	187	2.1	0.6	95
12/8/2024 4:30	0.5	3.1	166	0.2	1.3	152	1.8	0.6	76
12/8/2024 5:00	0.2	2.4	148	0.6	1.0	192	1.2	0.9	207
12/8/2024 5:30	0.2	0.2	64	0.2	1.9	205	0.9	1.0	190
12/8/2024 6:00	0.2	0.8	121	0.2	1.9	208	1.2	0.7	181
12/8/2024 6:30	0.2	3.8	205	2.1	2.8	214	1.3	1.2	185
12/8/2024 7:00	0.2	2.7	195	0.2	1.6	195	1.8	0.8	165
12/8/2024 7:30	0.2	3.2	192	0.2	2.3	194	2.1	1.3	205
12/8/2024 8:00	0.2	3.8	193	0.2	2.8	198	2.5	1.7	198
12/8/2024 8:30	0.2	3.1	195	0.2	2.1	212	1.5	1.1	178
12/8/2024 9:00	0.2	2.6	181	0.2	1.8	205	1.7	1.4	169
12/8/2024 9:30	0.2	3.4	186	0.2	2.8	221	0.6	2.5	222
12/8/2024 10:00	0.2	4.2	203	0.6	3.5	224	0.2	2.3	234
12/8/2024 10:30	0.2	3.6	233	1.1	4.6	250	0.2	2.2	226
12/8/2024 11:00	0.4	4.6	205	0.8	5.0	250	0.2	2.4	224
12/8/2024 11:30	0.5	5.5	212	0.6	5.8	241	0.2	2.7	226
12/8/2024 12:00	0.4	6.2	227	0.6	6.5	239	0.2	4.4	219
12/8/2024 12:30	0.2	6.7	216	0.5	6.4	235	0.2	3.0	231
12/8/2024 13:00	0.2	6.9	215	0.4	5.9	231	0.2	2.7	233
12/8/2024 13:30	0.2	8.3	224	0.5	6.8	229	0.5	3.4	222
12/8/2024 14:00	0.2	7.3	239	0.5	7.3	245	0.2	4.5	239
12/8/2024 14:30	0.2	6.5	234	0.6	6.7	244	0.2	4.5	242
12/8/2024 15:00	0.2	8.5	221	0.6	7.3	239	0.2	3.0	243
12/8/2024 15:30	0.2	10.1	222	0.6	8.6	236	0.2	4.7	231
12/8/2024 16:00	0.2	9.1	227	0.6	8.4	235	0.5	3.0	234
12/8/2024 16:30	0.2	7.5	207	0.6	5.9	229	0.7	3.0	225
12/8/2024 17:00	0.2	7.1	206	0.7	4.5	224	0.7	2.9	230
12/8/2024 17:30	0.2	4.6	200	0.6	2.6	222	0.6	2.7	222
12/8/2024 18:00	0.2	5.9	201	0.2	3.1	210	1.4	2.3	216
12/8/2024 18:30	0.2	5.9	199	0.2	3.7	215	1.9	2.4	205
12/8/2024 19:00	0.2	6.1	204	0.2	3.6	222	0.8	2.7	221
12/8/2024 19:30	0.2	4.2	203	0.2	2.6	220	0.9	1.5	220
12/8/2024 20:00	0.2	4.7	198	0.2	2.6	211	2.7	1.4	209
12/8/2024 20:30	0.2	3.6	195	0.2	2.3	207	2.2	1.2	195
12/8/2024 21:00	0.2	2.7	192	0.2	1.7	184	1.5	0.8	163
12/8/2024 21:30	0.4	2.0	170	0.2	1.3	182	0.4	0.8	205
12/8/2024 22:00	0.2	1.9	188	0.2	1.3	178	0.2	0.9	186
12/8/2024 22:30	0.2	1.8	185	0.2	1.1	185	0.4	0.7	202
12/8/2024 23:00	0.4	0.8	150	0.2	1.1	174	0.2	0.8	188
12/8/2024 23:30	0.5	1.1	222	0.2	0.5	295	0.2	0.4	192
12/9/2024 0:00	0.2	0.9	216	0.2	0.8	249	0.2	0.8	181

AQS Null Data Codes	
Qualifier Code	Item Description
AB	TECHNICIAN UNAVAILABLE
AC	CONSTRUCTION/REPAIRS IN AREA
AD	SHELTER STORM DAMAGE
AE	SHELTER TEMPERATURE OUTSIDE LIMITS
AI	INSUFFICIENT DATA (CAN'T CALCULATE)
AM	MISCELLANEOUS VOID
AN	MACHINE MALFUNCTION
AO	BAD WEATHER
AP	VANDALISM
AS	POOR QUALITY ASSURANCE RESULTS
AT	CALIBRATION
AU	MONITORING WAIVED
AV	POWER FAILURE (POWR)
AW	WILDLIFE DAMAGE
AX	PRECISION CHECK (PREC)
AY	Q C CONTROL POINTS (ZERO/SPAN)
BA	MAINTENANCE/ROUTINE REPAIRS
BB	UNABLE TO REACH SITE
BC	MULTI-POINT CALIBRATION
BD	AUTO CALIBRATION
BE	BUILDING/SITE REPAIR
BF	PRECISION/ZERO/SPAN
BJ	OPERATOR ERROR
BK	SITE COMPUTER/DATA LOGGER DOWN
BL	Q C AUDIT (AUDT)
EC	EXCEED CRITICAL CRITERIA